


# Configuration proposal Anesthesia Basic ANST

## Configuration description:

OndaScope400 with Service Head 400  
1 x shelf 520 mm


1. Brake system: friktion
2. Action space\*: ---
3. Weights and pay loads  
remaining net pay load: 226 kg  
max. pendant pay load: 250 kg  
vertical force as configured: 3317 N
4. Remaining diameter: 66 %

\* reference: centre of main bearing to centre of shelf

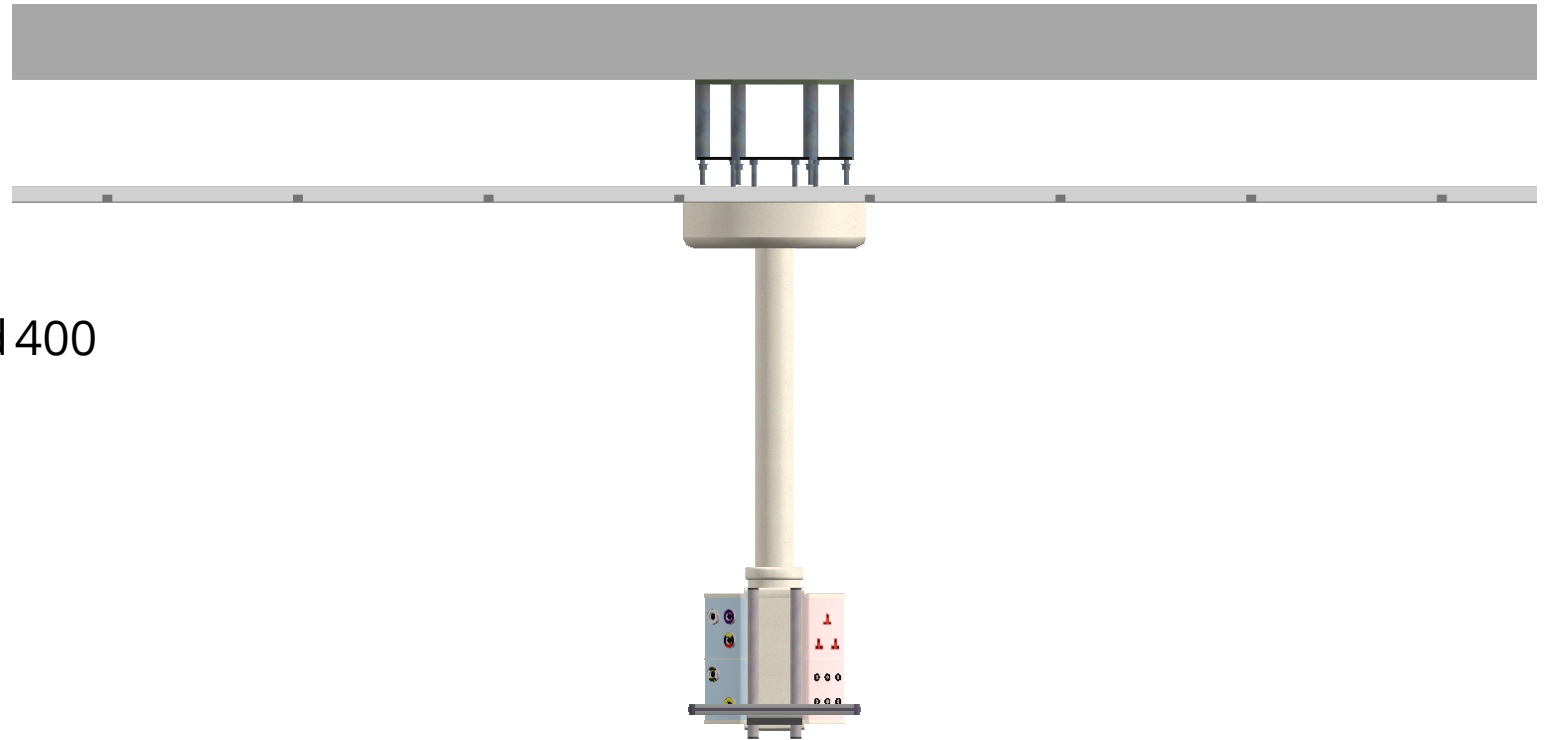

# Configuration proposal Anesthesia Basic ANST


Side view right

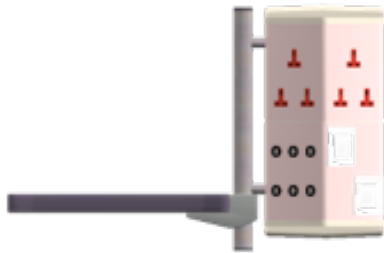

Front view



Side view left

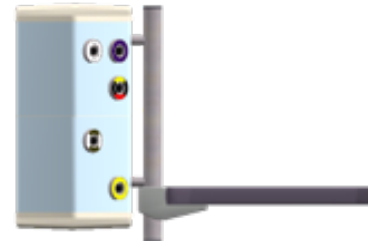

Back



Number of service components											
O <sub>2</sub>	Air 4/5	N <sub>2</sub> O	Vac	CO <sub>2</sub>	N <sub>2</sub>	AGSS	Air 8/ Air- motor	Electrical sockets	Earth bonding sockets	Double RJ45	Data prep.
1	1	1	1			1		6	6		2
Phoenix P3 British Standard (ISO)								Wands- worth			