



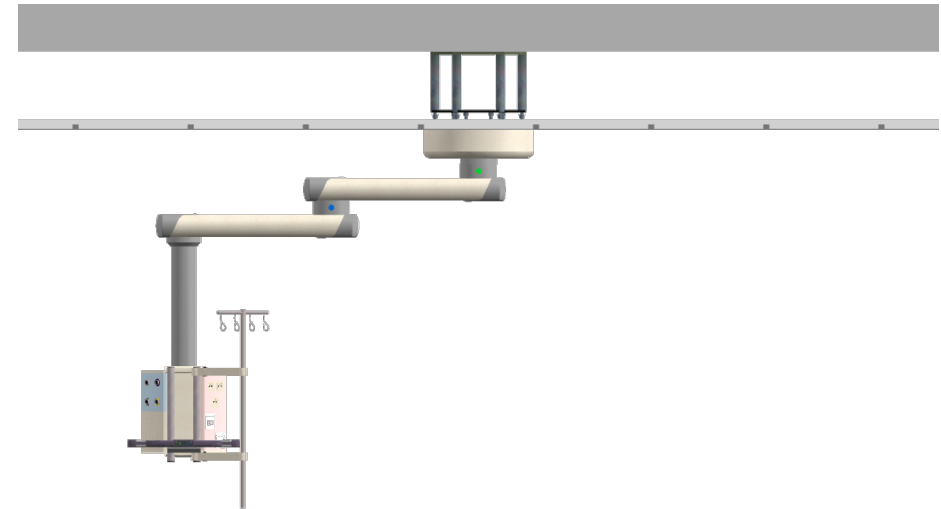

# Configuration proposal Anesthesia (AN2)

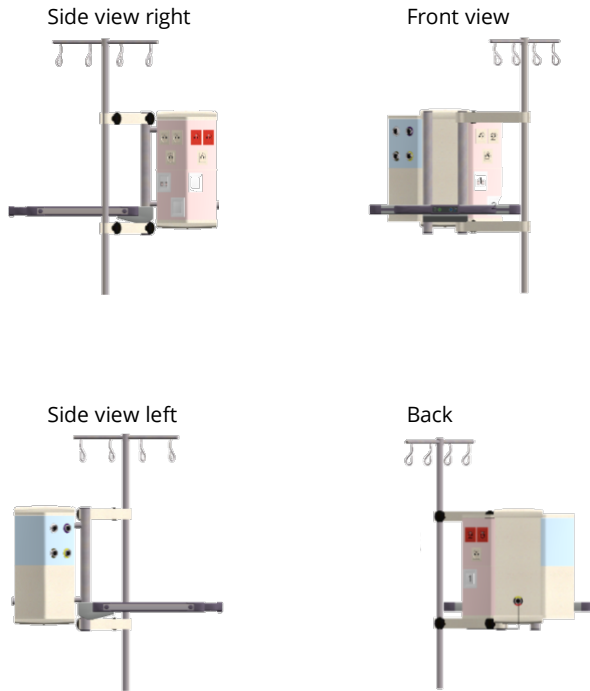

Configuration description:  
 MediBoom®Air 800/800 with Service Head 400  
 1 x Shelf 520 mm, 1 x IV pole

1. Brake system: Pneumatic
2. Action space\*: >4,000 mm
3. Weights and Pay Loads  
 Remaining Net Pay Load: 142 kg  
 Max. pendant pay load: 180 kg  
 Vertical force as configured: 3025 N
4. Remaining Diameter: 74 %

				Number of service components							
O <sub>2</sub>	Air 4/5	N <sub>2</sub> O	Vac	CO <sub>2</sub>	N <sub>2</sub>	AGSS	Air 8/ Air- motor	Electrical sockets	Earth bonding sockets	Double RJ45	Data prep.
1	1	1	1			1		6	6	1	2
DKD AFNOR (Norme francaise)								Legrand			

\* reference: centre of main bearing to centre of shelf




# Configuration proposal Anesthesia (AN2)

Side view right




Front view

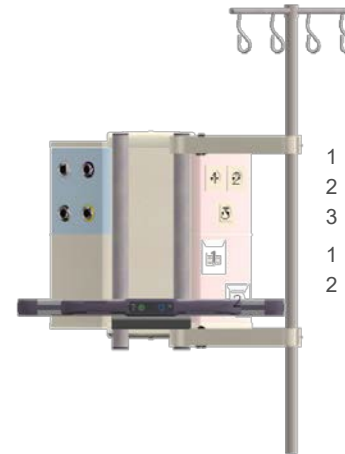


- O2 1
- N2O 2
- AIR5 3
- VAC 4

- 1 White
- 2 White
- 3 White
- 1 2x Cat6 IDC
- 2 Preparation

Side view left

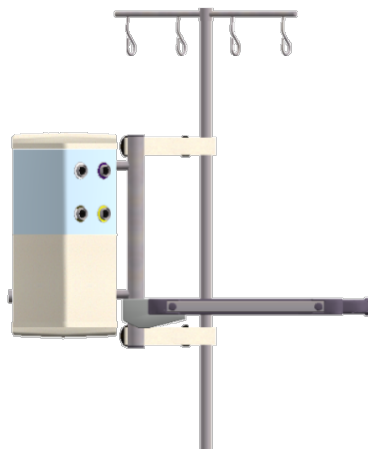

Back

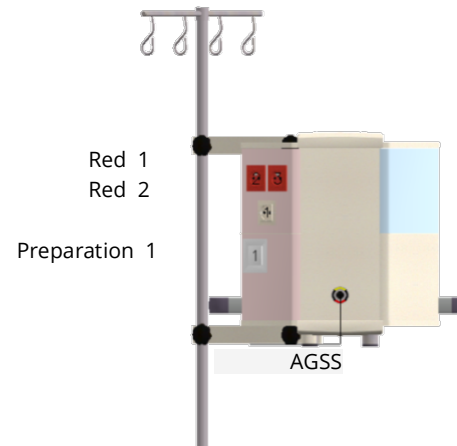

- Red 1
- Red 2

Preparation 1

AGSS