



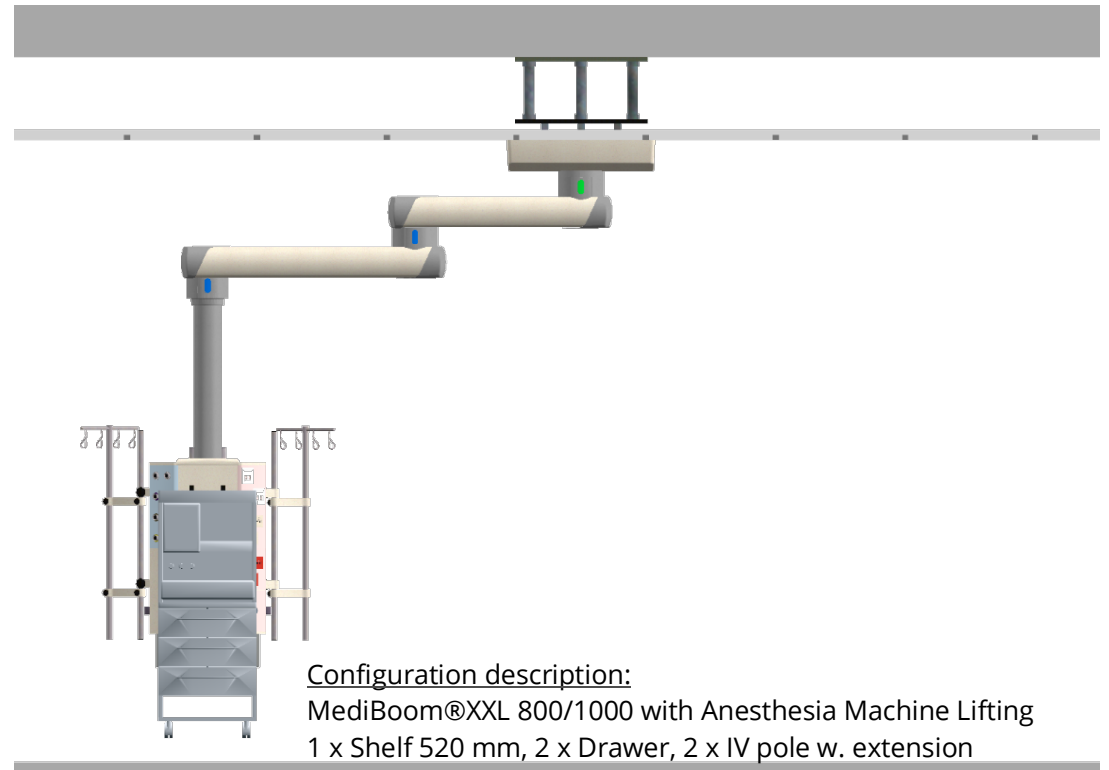

Configuration proposal Anesthesia (AN5)

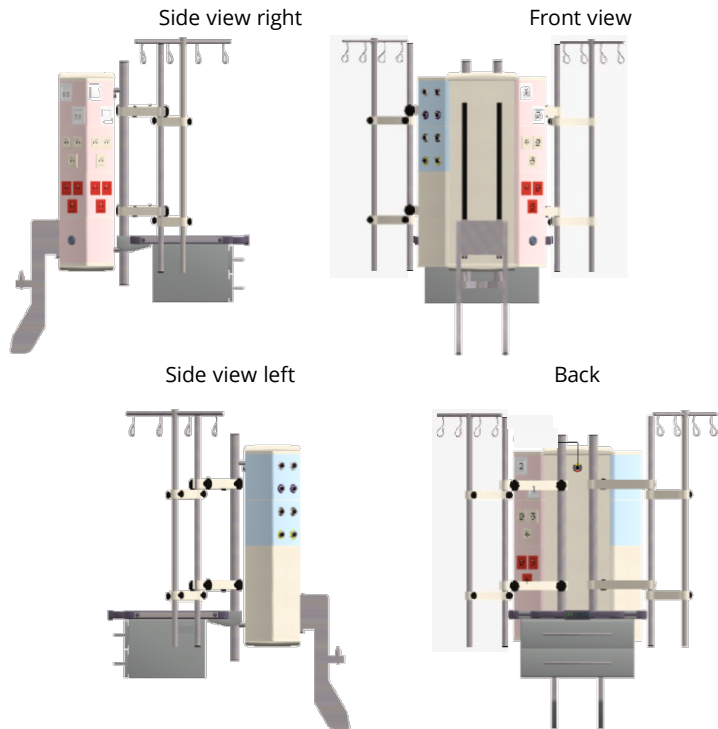

1. Brake system: Electromagnetic
2. Action space*: >4,400 mm
3. Weights and Pay Loads
 Remaining Net Pay Load: 241 kg
 Max. pendant pay load: 340 kg
 Vertical force as configured: 5684 N
4. Remaining Diameter: 68 %

Number of service components											
O ₂	Air 4/5	N ₂ O	Vac	CO ₂	N ₂	AGSS	Air 8/ Air- motor	Electrical sockets	Earth bonding sockets	Double RJ45	Data prep.
2	2	2	2			1		12	12	2	2
DKD AFNOR (Norme francaise)								Legrand			

* reference: centre of main bearing to centre of shelf




Configuration proposal Anesthesia (AN5)

Side view right



Front view

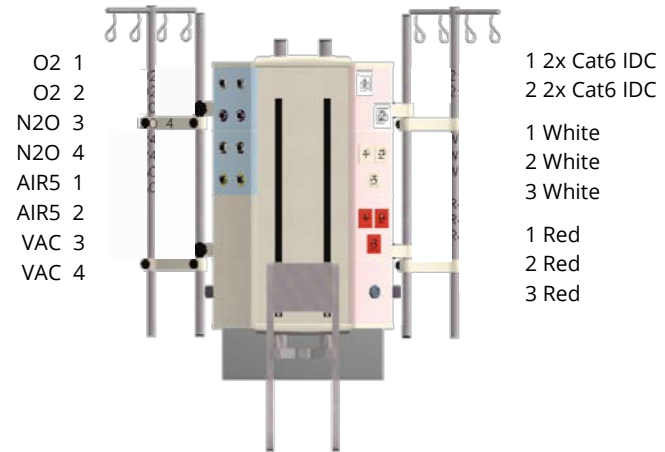

Side view left



Back

