



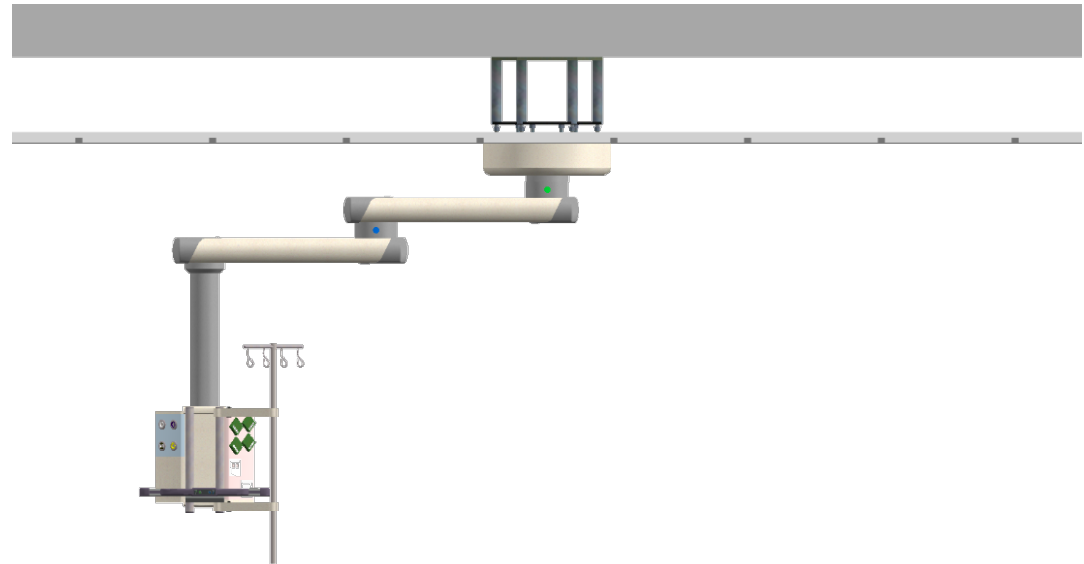

Configuration proposal Anesthesia (AN2)

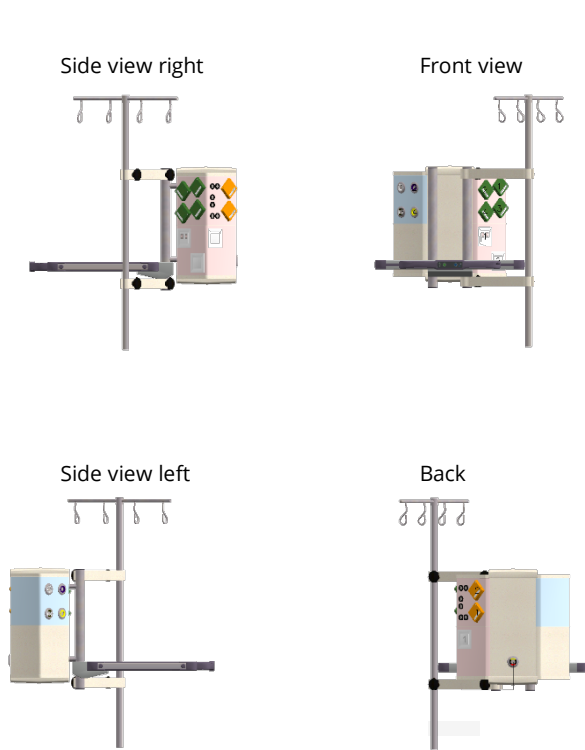

Configuration description:
 MediBoom®Air 800/800 with Service Head 400
 1 x Shelf 520 mm, 1 x IV pole

1. Brake system: Pneumatic
2. Action space*: >4,000 mm
3. Weights and Pay Loads
 Remaining Net Pay Load: 139 kg
 Max. pendant pay load: 180 kg
 Vertical force as configured: 3025 N
4. Remaining Diameter: 67 %


Number of service components											
O ₂	Air 4/5	N ₂ O	Vac	CO ₂	N ₂	AGSS	Air 8/ Air- motor	Electrical sockets	Earth bonding sockets	Double RJ45	Data prep.
1	1	1	1			1		6	6	1	2
Greggersen Forano DIN Standard								PEHA			

* reference: centre of main bearing to centre of shelf




Configuration proposal Anesthesia (AN2)

Side view right

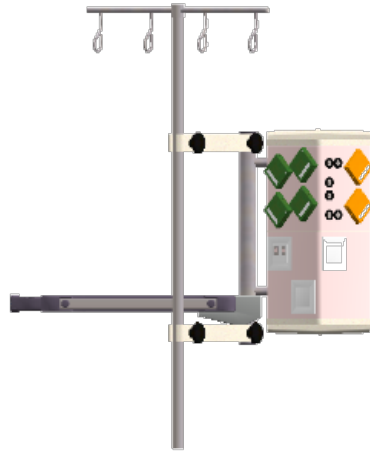


Front view

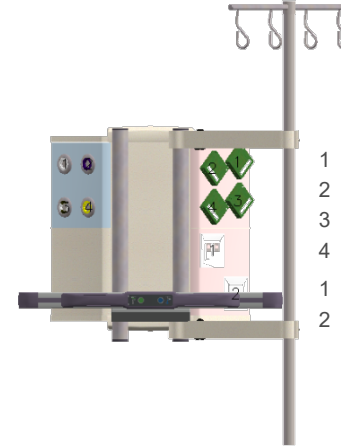

- O2 1
- N2O 2
- AIR5 3
- VAC 4

- 1 Green
- 2 Green
- 3 Green
- 4 Green
- 1 2x Cat6 IDC
- 2 Preparation

Side view left

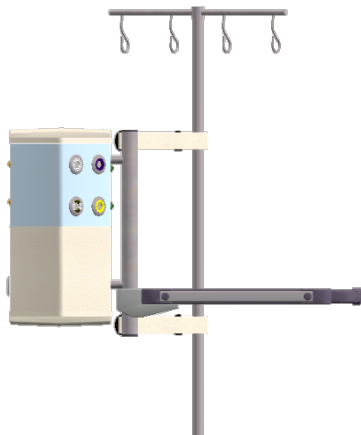

Back

