





# Configuration proposal Anesthesia (AN5)

Side view right

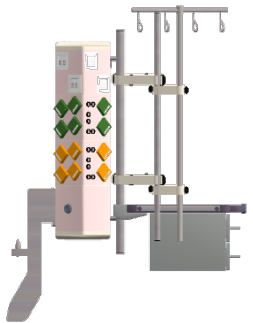



Front view

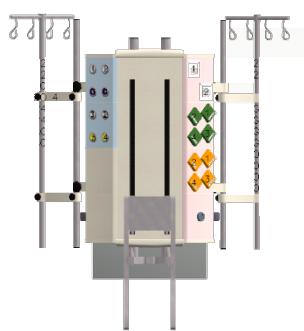

Side view left



Back

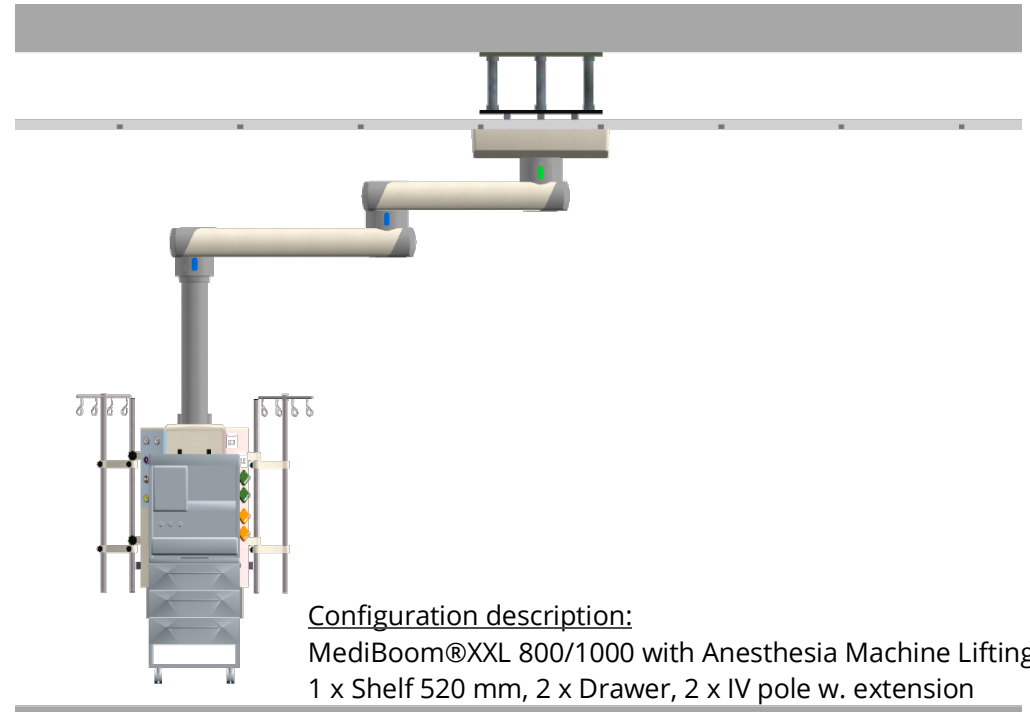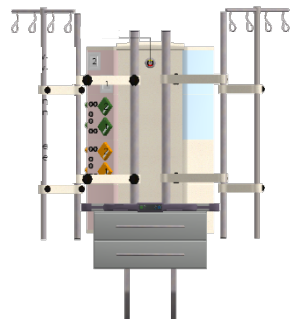

Configuration description:

MediBoom@XXL 800/1000 with Anesthesia Machine Lifting  
 1 x Shelf 520 mm, 2 x Drawer, 2 x IV pole w. extension

1. Brake system: Electromagnetic
2. Action space\*: >4,400 mm
3. Weights and Pay Loads  
 Remaining Net Pay Load: 235 kg  
 Max. pendant pay load: 340 kg  
 Vertical force as configured: 5684 N
4. Remaining Diameter: 52 %


Number of service components											
O <sub>2</sub>	Air 4/5	N <sub>2</sub> O	Vac	CO <sub>2</sub>	N <sub>2</sub>	AGSS	Air 8/ Air- motor	Electrical sockets	Earth bonding sockets	Double RJ45	Data prep.
2	2	2	2			1		12	12	2	2
Greggersen Forano DIN Standard								PEHA			

\* reference: centre of main bearing to centre of shelf




# Configuration proposal Anesthesia (AN5)

Side view right

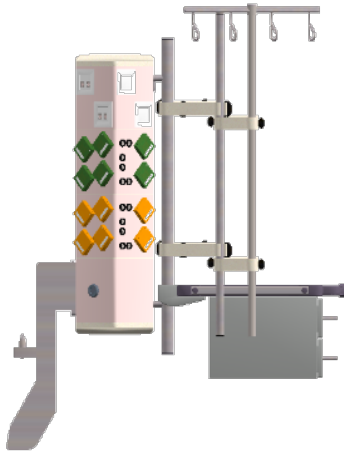

Front view

- |        |               |
|--------|---------------|
| O2 1   | 1 2x Cat6 IDC |
| O2 2   | 2 2x Cat6 IDC |
| N2O 3  | 1 Green       |
| N2O 4  | 2 Green       |
| AIR5 1 | 3 Green       |
| AIR5 2 | 4 Green       |
| VAC 3  | 1 Orange      |
| VAC 4  | 2 Orange      |
|        | 3 Orange      |
|        | 4 Orange      |

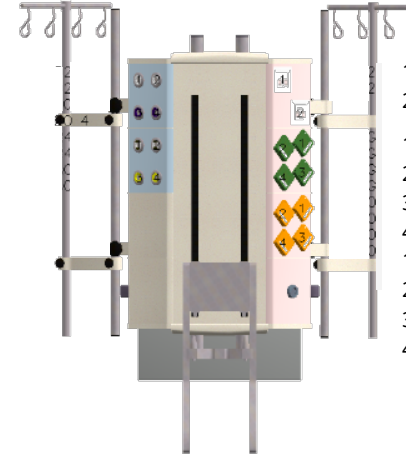

Side view left



Back

- |               |
|---------------|
| Preparation 1 |
| Preparation 2 |
| Green 3       |
| Green 4       |
| Orange 1      |
| Orange 2      |

