


Configuration proposal Anesthesia Basic ANST

Configuration description:

OndaScope400
with Service Head 400
1 x shelf 520 mm


1. Brake system: friktion
2. Action space*: ---
3. Weights and pay loads:
 - remaining net pay load: 222 kg
 - max. pendant pay load: 250 kg
 - vertical force as configured: 3317 N
4. Remaining diameter: 70 %

* reference: centre of main bearing to centre of shelf

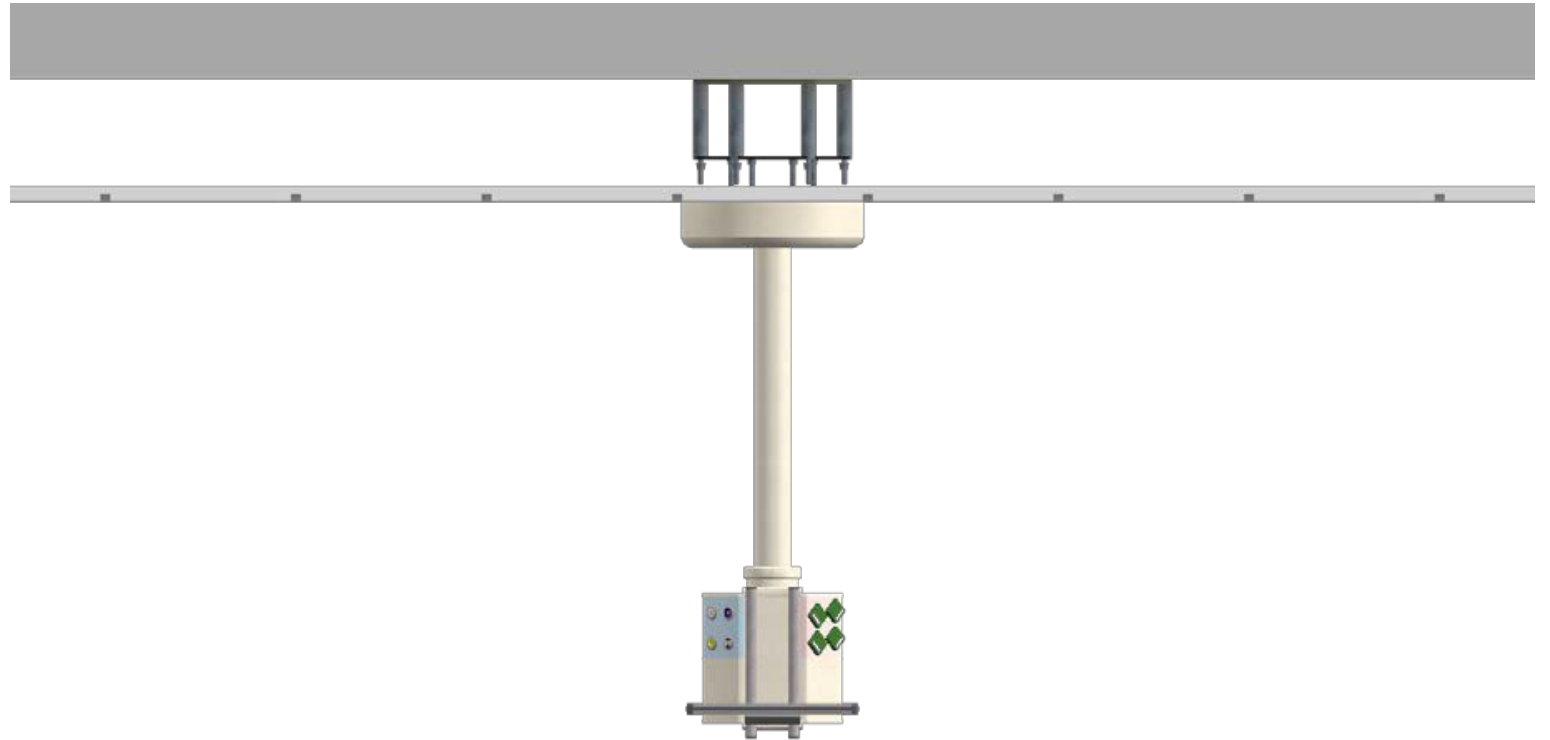


Configuration proposal Anesthesia Basic ANST

Side view right

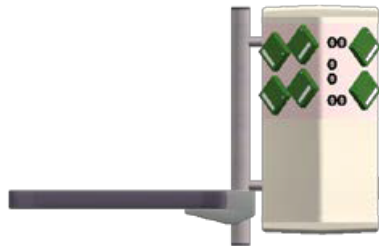

Front view

O2 1
N2O 2
Air 4 3
VAC 4



Green 1
Green 2
Green 3
Green 4

Side view left



Back

Green 1
Green 2



AGSS

| Number of service components | | | | | | | | | | | |
|------------------------------|---------|------------------|-----|-----------------|----------------|------|-------------------------|-----------------------|-----------------------------|----------------|------------|
| O ₂ | Air 4/5 | N ₂ O | Vac | CO ₂ | N ₂ | AGSS | Air 8/ Air- motor | Electrical sockets | Earth bonding sockets | Double RJ45 | Data prep. |
| 1 | 1 | 1 | 1 | | | 1 | | 6 | 6 | | 2 |
| DIN Standard | | | | | | | | | | | |