

# Configuration proposal General Surgery Basic CHST

## Configuration description:


OndaScope400

with Service Head 400

1 x shelf 520 mm


1. Brake system: friktion
2. Action space\*: ---
3. Weights and pay loads:
  - remaining net pay load: 224 kg
  - max. pendant pay load: 250 kg
  - vertical force as configured: 3317 N
4. Remaining diameter: 86%

\* reference: centre of main bearing to centre of shelf

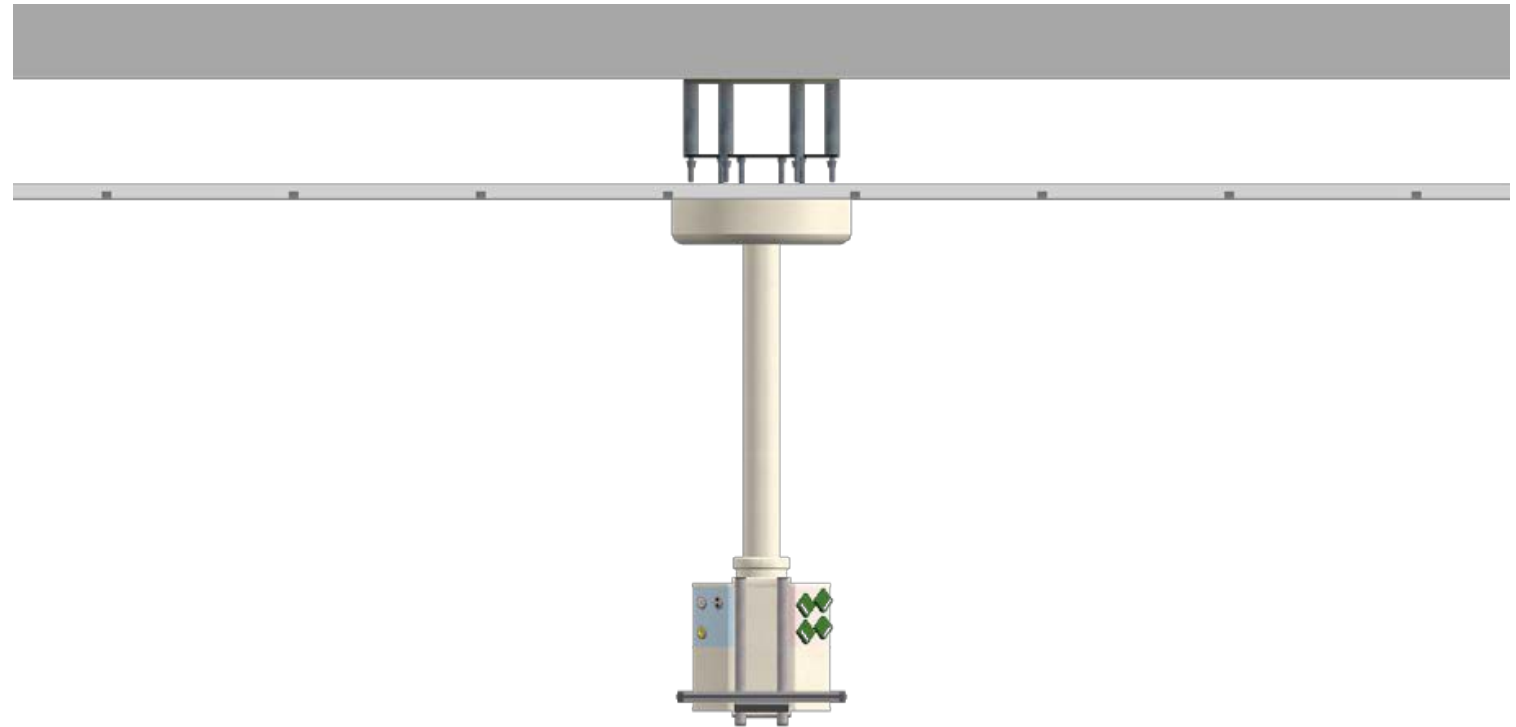


# Configuration proposal General Surgery Basic CHST

Side view right

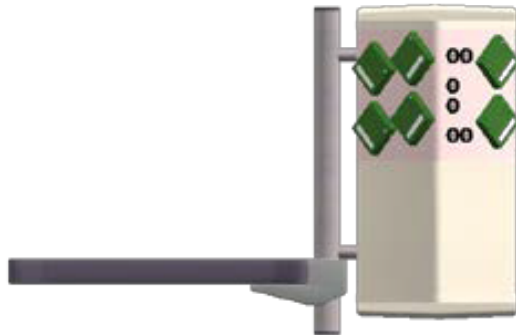

Front view

O2 1  
Air4 2  
VAC 3

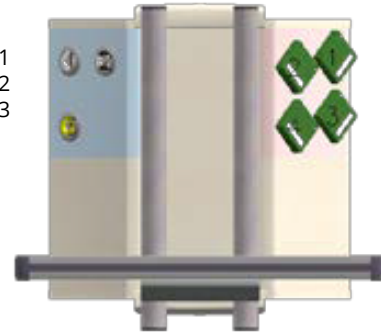


Green 1  
Green 2  
Green 3  
Green 4

Side view left



Back

Green 1  
Green 2

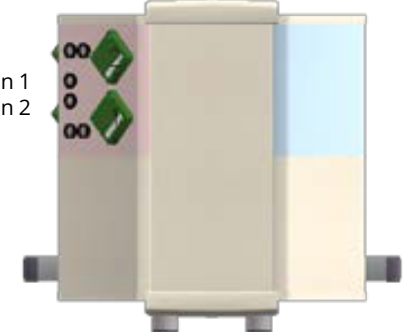

Number of service components											
O <sub>2</sub>	Air 4/5	N <sub>2</sub> O	Vac	CO <sub>2</sub>	N <sub>2</sub>	AGSS	Air 8/ Air- motor	Electrical sockets	Earth bonding sockets	Double RJ45	Data prep.
1	1		1					4	4		
DIN Standard											